

# ADMS 6 Buildings Validation

## Warehouse Fires Wind Tunnel Experiments

Cambridge Environmental Research Consultants  
April 2023


### 1 Introduction

In 1996, results from the CERC Atmospheric Dispersion Model, ADMS 2 were validated against experimental wind tunnel data of dispersion from chemical warehouse fires [1]. The original experimental data used to validate the model were presented in a Building Research Establishment Client Report [2]. Here, results from the latest model version (ADMS 6.0.0.1, henceforth ADMS 6.0) are validated against these experimental data, and corresponding results from the previous model version (ADMS 5.2.0.0, henceforth ADMS 5.2) are also presented.

Section 2 describes the experimental set up used in the wind tunnel experiments. Section 3 describes the exact input used for the ADMS runs. The results are presented in Section 4 and a summary of the results is given in Section 5.

### 2 Experimental set up

For full details of the experimental set up used, please refer to the BRE Client Report [2]. The experiments were carried out at model scale, which was taken to be 1/150 of a full scale sized warehouse. Two warehouse dimensions were used for comparison purposes: a large and a small warehouse. **Figure 1** shows the building shapes used.

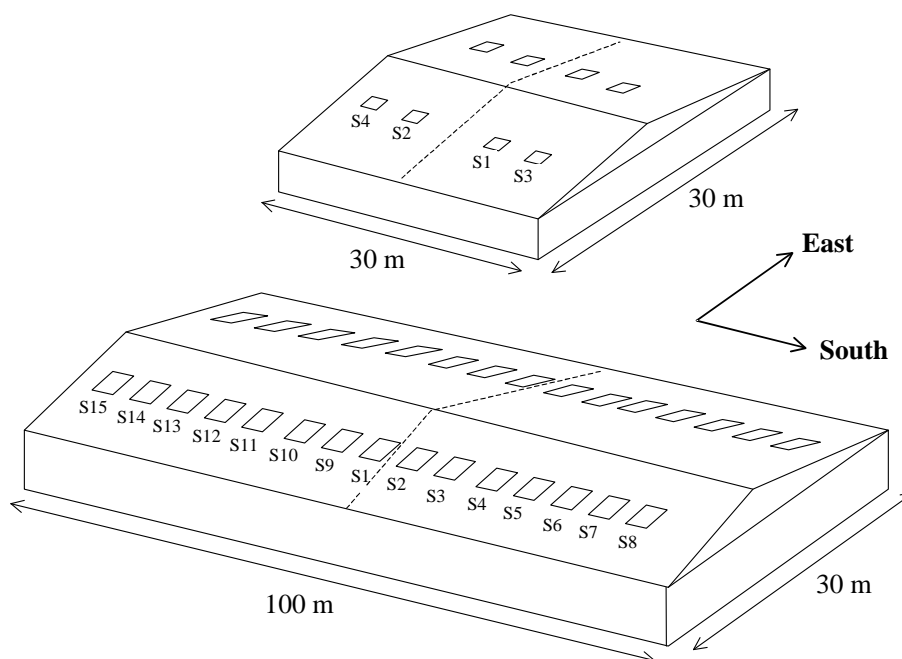

**Figure 1** – The small building shape (top) and large building shape (bottom).

The roof openings were taken as the source of the smoke from the warehouse fire and the wind was taken as to be coming from the West. For both buildings, different numbers of roof openings were considered in separate experiments; that is, for the large building, the smoke was taken to come out of 1, 4, 9 and 15 openings, and for the small building, out of 1, 2 and 4 openings.

Three different buoyancy cases were considered. These are named as *Cases S, W and X*, and are summarized in **Table 1** (which is derived from to Table 2 in [2]). Here, the buoyancy flux parameter  $F_b$  is defined as

$$F_b = \frac{F}{U^3 L},$$

where  $U$  is the wind speed at reference height (taken to be the top of the building),  $L$  is the physical length scale of the experiment (taken to be the height of the building).

$F$  is the buoyancy flux defined by

$$F = g \frac{\Delta\rho}{\rho_a} \frac{V}{\pi},$$

where  $g$  is the acceleration due to gravity,  $\rho_a$  is the ambient gas density,  $\rho$  is the density of the smoke ( $\Delta\rho = \rho_a - \rho$ ), and  $V$  is the volume emission rate of the discharged fire plume.

The momentum flux parameter  $F_m$  is defined as

$$F_m = \frac{\rho}{\rho_a} \frac{V w}{U^2 L^2},$$

where  $w$  is the fire plume gas exit velocity.

Case	Buoyancy flux parameter $F_b$	Momentum flux parameter $F_m$	Model wind speed $U$	Source diameter	Gas volume emission rate $V$
S	0.0	0.000	1.0	13	1.0
W	0.1	0.116	0.5	13	19.6
X	0.3	0.400	0.4	13	29.8

**Table 1** – Experimental set up parameters (model scale).  $U$  in m/s, diameter in mm, volume emission rate in l/min.

#### Note

1. The exit velocities/volume emission rates entered into the model runs are calculated from the values in the gas volume emission rates indicated in **Table 1**, not from the momentum flux parameter  $F_m$  given in the table. There is a slight inconsistency here, in particular for Case S where a momentum flux of zero must correspond to a volume emission rate of zero. The values of  $F_m$  and  $V$  agree to within about 5 % for Cases W and X.

2. The relationship between lengths for the model  $L_{\text{mod}}$  and full scale  $L_{fs}$  is

$$L_{fs} = 150 L_{\text{mod}},$$

which leads to the following relationship between model  $U_{\text{mod}}$  and full scale  $U_{fs}$  velocities:

$$U_{fs} = \sqrt{150} U_{\text{mod}}.$$

### 3 Input data

This section summarizes the data input into the ADMS model.

Note that all parameters given are for the full scale set up. Five sets of data are discussed: building data, source data, roughness length, meteorological data and output grid.

#### 3.1 Buildings

One building is modelled and the height is taken to be 10 m, which is the height of the building to the eaves. Other building parameters for the large and small building are given in **Table 2**.

Building	Height (m)	Length (m)	Width (m)	Angle (°)	Centre (m)
large	10	100	30	0	(-15, 0)
small	10	30	30	0	(-15, 0)

**Table 2** – Building dimensions, orientation and location. The angle is the angle between north and the building length measured clockwise from north.

#### 3.2 Source parameters

The roof openings (sources) are shown in **Figure 1**. The locations of the 15 sources on the large building are given in **Table 3** and those of the 4 sources on the small building are given in **Table 4**.

Source	Location	Source	Location
S1	(-22.50, 0.00)	S9	(-22.50, 6.37)
S2	(-22.50, -6.37)	S10	(-22.50, 12.74)
S3	(-22.50, -12.74)	S11	(-22.50, 19.11)
S4	(-22.50, -19.11)	S12	(-22.50, 25.38)
S5	(-22.50, -25.38)	S13	(-22.50, 31.85)
S6	(-22.50, -31.85)	S14	(-22.50, 38.22)
S7	(-22.50, -38.22)	S15	(-22.50, 44.59)
S8	(-22.50, -44.59)		

**Table 3** – Source locations for the large building.

Source	Location
S1	(-22.500, -3.195)
S2	(-22.500, 3.195)
S3	(-22.500, -9.585)
S4	(-22.500, 9.585)

**Table 4** – Source locations for the small building.

For the large building, four different cases were considered: 1 roof opening (S1), 4 roof openings (S1-S3 and S9), 9 roof openings (S1-S5 and S9-S12) and 15 roof openings (S1-S15). For each case, an emission rate of 1 g/s was taken. That is for one opening, the source emission rate was 1 g/s whereas for 4 openings, each source has an emission rate of 0.25 g/s. Similarly, the volume flow rate/gas exit velocity (which varies for each of the Cases S, W and X) is divided

equally between the sources. Sources are taken to be circular.

For the small building, three different cases were considered: 1 roof opening (S1), 2 roof openings (S1-S2) and 4 roof openings (S1-S4). Emission rates and volume flow rates were divided equally between the roof openings, as for the large building.

The remaining source input parameters are summarized in **Table 5**.

Case	Height (m)	Diameter (m)	Exit volume rate (m <sup>3</sup> /s)	Gas density (kg/m <sup>3</sup> )	Emission rate (g/s)
S	10	1.95	4.59	1.225	1
W	10	1.95	90.02	0.222	1
X	10	1.95	136.90	0.212	1

**Table 5** – Source parameters.

### 3.3 Roughness length

The roughness length was taken to be 0.3 m.

### 3.4 Meteorological data

The meteorological data are summarized in **Table 6**.

The definition of the surface sensible heat flux  $F_{\theta}$  is not discussed here as it suffices to say that a value of  $F_{\theta} = 0 \text{ W/m}^2$  corresponds to neutral atmospheric conditions (Pasquill-Gifford stability category D).

The height of the recorded wind was taken in all cases to be 10 m.

Case	Wind speed (m/s)	Wind direction (°)	Boundary-layer height (m)	Surface sensible heat flux (W/m <sup>2</sup> )
S	12.25	270	82.5	0
W	6.12	270	82.5	0
X	4.90	270	82.5	0

**Table 6** – Meteorological data.

### 3.5 Output grid

The output considered was at 15 locations downstream of the centre of building at locations  $x = 9.375, 18.75, 37.5, 75, 112.5$  and then at 37.5 m intervals until  $x = 487.5$  m.

## 4 Results

For each of the models (ADMS 5.2 and ADMS 6.0), there are 12 sets of experimental results for the large building and 9 sets for the small building. For each experiment, 15 data points are compared. The best way to display results such as these is statistically. These statistics were calculated using the Model Evaluation toolkit v5.2 [4].

The statistics are presented separately for the large and small building, and for buoyancy cases (S, W and X) and roof openings (1, 4, 9 and 15 for the large building; 1, 2 and 4 for the small

building) in addition to the overall performance statistics.

As the experiment was performed at model scale, and the ADMS results are at full scale, statistics are calculated from the non-dimensional parameter  $K$  defined by

$$K = CUL^2/Q$$

where  $C$  is the concentration in  $\text{g/m}^3$ ,  $Q$  is the emission rate in  $\text{g/s}$ , and  $U$  and  $L$  are as defined in the Section 2.


#### 4.1 Large building

**Figure 2** gives the 5<sup>th</sup>, 25<sup>th</sup>, 50<sup>th</sup>, 75<sup>th</sup> and 95<sup>th</sup> percentiles of the ratio modelled to experimental values, for all runs divided into buoyancy cases.


**Figure 3** gives shows the same set of results, but separated into number of roof openings.

Other statistics such as mean, variance (Sigma), bias, normalized mean square error (NMSE), correlation (Cor), values within a factor of 2 of the experimental values (Fa2), fractional bias (Fb) and fractional standard deviation (Fs) are presented in the following tables, as output directly from the Model Evaluation Toolkit.

**Table 7** gives the statistics divided into the buoyancy cases and **Table 8** gives the values divided into the number of openings. **Table 9** gives the summary statistics.

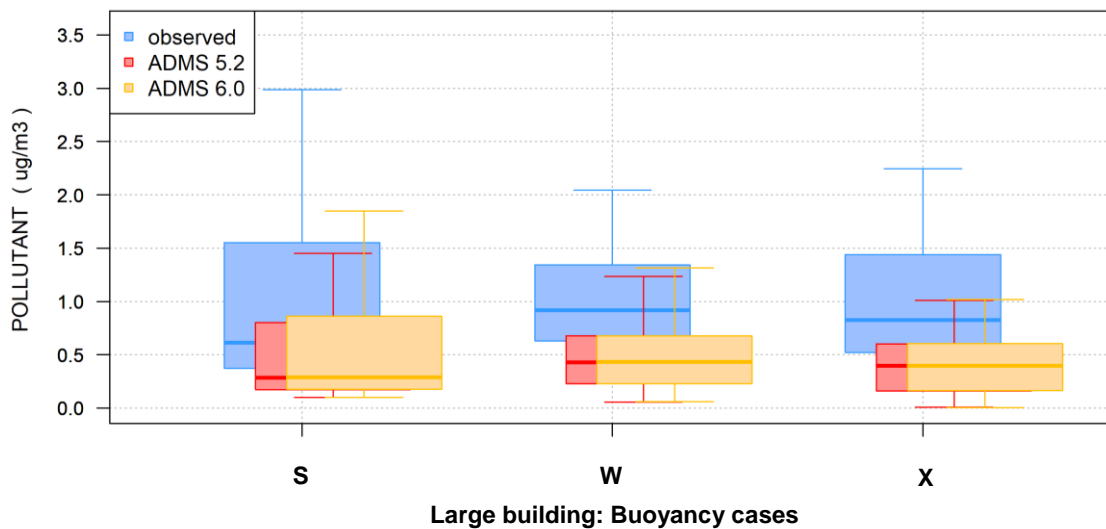

**Figure 2** – Box and whisker plot of the results for the large building: buoyancy cases.

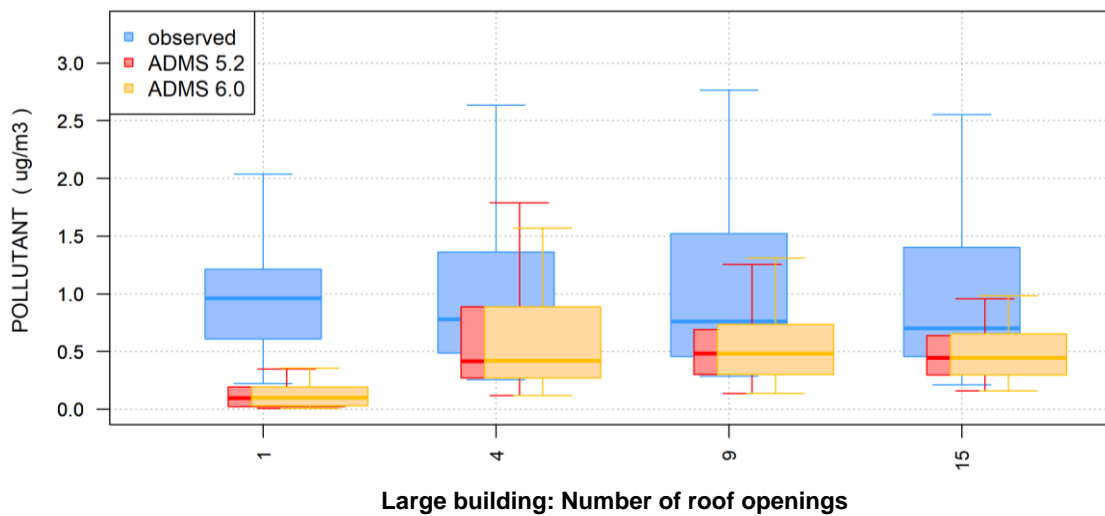

**Figure 3** – Box and whisker plot of the results for the large building: roof openings.

Case	Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
S	BRE (obs.)	1.00	0.83	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.51	0.48	-0.49	0.79	0.943	0.383	-0.641	-0.546
	ADMS 6.0	0.57	0.53	-0.43	0.55	0.942	0.450	-0.553	-0.369
W	BRE (obs.)	1.00	0.49	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.49	0.37	-0.51	0.91	0.500	0.633	-0.678	-0.269
	ADMS 6.0	0.50	0.38	-0.50	0.88	0.512	0.633	-0.666	-0.249
X	BRE (obs.)	1.00	0.55	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.40	0.28	-0.60	1.63	0.281	0.433	-0.854	-0.649
	ADMS 6.0	0.41	0.28	-0.60	1.60	0.290	0.433	-0.847	-0.643

**Table 7** – Statistics for the large building: buoyancy cases S, W and X.

Case	Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
1	BRE (obs.)	1.00	0.60	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.21	0.36	-0.79	3.78	0.723	0.044	-1.301	-0.505
	ADMS 6.0	0.23	0.43	-0.77	3.20	0.742	0.067	-1.241	-0.331
4	BRE (obs.)	1.00	0.65	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.63	0.48	-0.37	0.46	0.800	0.533	-0.452	-0.291
	ADMS 6.0	0.66	0.55	-0.34	0.38	0.821	0.556	-0.410	-0.172
9	BRE (obs.)	1.00	0.65	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.54	0.29	-0.46	0.76	0.819	0.689	-0.598	-0.760
	ADMS 6.0	0.56	0.33	-0.44	0.67	0.825	0.711	-0.568	-0.662
15	BRE (obs.)	1.00	0.66	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.50	0.23	-0.50	1.04	0.741	0.667	-0.672	-0.969
	ADMS 6.0	0.51	0.25	-0.49	0.96	0.755	0.689	-0.647	-0.894


**Table 8** – Statistics for the large building: roof openings 1, 4, 9 and 15.

Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
BRE (obs.)	1.00	0.64	0.00	0.00	1.000	1.000	0.000	0.000
ADMS 5.2	0.47	0.39	-0.53	1.07	0.681	0.483	-0.721	-0.494
ADMS 6.0	0.49	0.43	-0.51	0.95	0.705	0.506	-0.683	-0.386


**Table 9** – Statistics for the large building.

### 4.2 Small building

**Figure 4** gives the 5<sup>th</sup>, 25<sup>th</sup>, 50<sup>th</sup>, 75<sup>th</sup> and 95<sup>th</sup> percentiles of the ratio of modelled to experimental values for all runs divided into buoyancy cases. **Figure 5** shows the same set of results, but separated into number of roof openings.

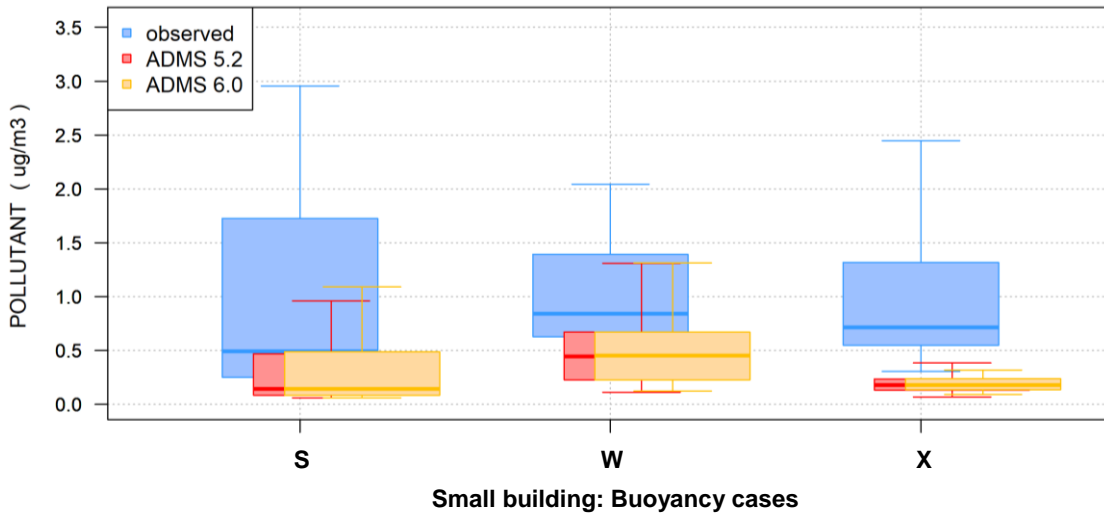

**Figure 4** – Box and whisker plot of the results for the small building: buoyancy cases.

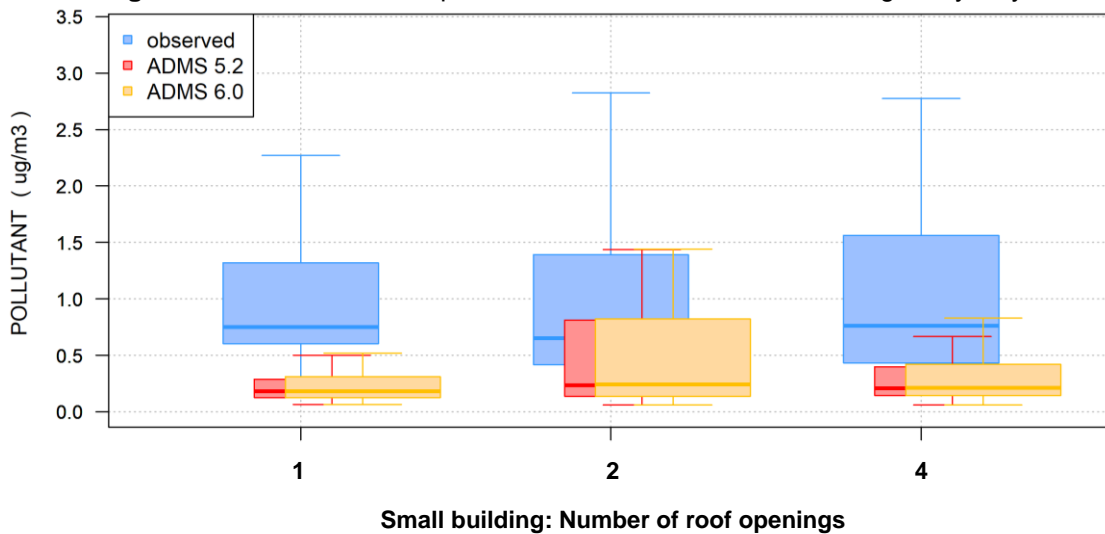

**Figure 5** – Box and whisker plot of the results for the small building: roof openings.

Other statistics such as mean, variance (Sigma), bias, normalized mean square error (NMSE), correlation (Cor), values within a factor of 2 of the experimental values (Fa2), fractional bias (Fb) and fractional standard deviation (Fs) are presented in the next tables, as output directly from the Model Evaluation Toolkit. **Table 10** gives the statistics divided into the buoyancy cases and **Table 11** gives the values divided into the number of openings. **Table 12** gives the summary statistics.

Case	Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
S	BRE (obs.)	1.00	0.94	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.31	0.32	-0.69	2.84	0.965	0.000	-1.051	-0.989
	ADMS 6.0	0.33	0.36	-0.67	2.42	0.968	0.000	-0.999	-0.901
W	BRE (obs.)	1.00	0.49	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.49	0.33	-0.51	1.04	0.299	0.556	-0.677	-0.391
	ADMS 6.0	0.50	0.33	-0.50	1.00	0.326	0.556	-0.667	-0.394
X	BRE (obs.)	1.00	0.69	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.27	0.33	-0.72	2.97	0.647	0.067	-1.139	-0.700
	ADMS 6.0	0.29	0.34	-0.71	2.79	0.642	0.111	-1.110	-0.682

**Table 10** – Statistics for the small building: buoyancy cases S, W and X.

Case	Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
1	BRE (obs.)	1.00	0.69	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.31	0.35	-0.69	2.22	0.829	0.066	-1.064	-0.643
	ADMS 6.0	0.32	0.37	-0.68	1.99	0.837	0.089	-1.023	-0.601
2	BRE (obs.)	1.00	0.78	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.46	0.38	-0.54	1.63	0.523	0.289	-0.747	-0.691
	ADMS 6.0	0.47	0.39	-0.53	1.50	0.566	0.311	-0.723	-0.672
4	BRE (obs.)	1.00	0.72	0.00	0.00	1.000	1.000	0.000	0.000
	ADMS 5.2	0.32	0.25	-0.68	2.49	0.694	0.267	-1.036	-0.952
	ADMS 6.0	0.33	0.27	-0.67	2.31	0.723	0.267	-1.013	-0.904

**Table 11** – Statistics for the small building: roof openings 1, 2 and 4.

Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
BRE (obs.)	1.00	0.73	0.00	0.00	1.000	1.000	0.000	0.000
ADMS 5.2	0.36	0.34	-0.64	2.05	0.649	0.207	-0.942	-0.727
ADMS 6.0	0.37	0.35	-0.63	1.88	0.679	0.222	-0.913	-0.694

**Table 12** – Statistics for the small building.

### 4.3 Both buildings

**Figure 6** gives the 5<sup>th</sup>, 25<sup>th</sup>, 50<sup>th</sup>, 75<sup>th</sup> and 95<sup>th</sup> percentiles of the modelled/experimental values, for all runs and both buildings. Other statistics such as mean, variance (Sigma), bias, normalized mean square error (NMSE), correlation (Cor), values within a factor of 2 of the experimental values (Fa2), fractional bias (Fb) and fractional standard deviation (Fs) are presented in **Table 13**, as output directly from the Model Evaluation Toolkit.



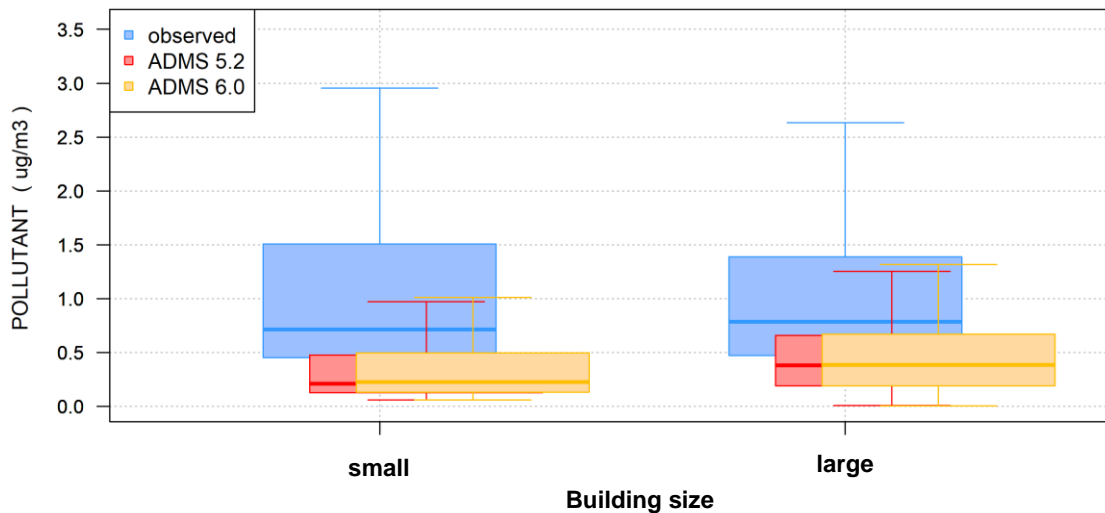


Figure 6 – Box and whisker plot of the results for both buildings.

Data	Mean	Sigma	Bias	NMSE	Cor	Fa2	Fb	Fs
BRE (obs.)	1.00	0.68	0.00	0.00	1.000	1.000	0.000	0.000
ADMS 5.2	0.42	0.37	-0.58	1.43	0.654	0.365	-0.812	-0.587
ADMS 6.0	0.44	0.41	-0.56	1.29	0.678	0.384	-0.777	-0.507

Table 13 – Statistics for both buildings.

## 5 Summary

Table 13 gives the summary results for both buildings. The model tends to under-predict the measured concentrations in general. The correlation between modelled and observed values is reasonable ( $>0.6$ ).

Results indicate that, with the exception of the ‘1 opening’ case, the large building results agree better with modelled values than the smaller building (compare Figures 3 and 5).

One would expect results to become less accurate as buoyancy increases from Cases S to W to X. This is because with the increasingly buoyant cases, the plume may pass through the top of the boundary layer and reach the top of the wind tunnel, and then may be reflected back. The behaviour of a plume in the atmospheric boundary layer is different – the fraction of the plume re-entering the boundary layer depends on the temperature inversion at the top of the boundary layer. These experiments demonstrate this – Figures 2 and 4 show how the spread of modelled/observed results increases with buoyancy. The value of correlation between the modelled and observed results also follows this pattern, as can be seen in Tables 7 and 10.

The differences between ADMS 5.2 and ADMS 6.0 are generally small, although ADMS 6.0 performs slightly better. In ADMS 6.0, the ground-level plume emanating from recirculation region is modelled as a line source rather than a point source, with an initial concentration that is better matched to the uniform concentration of the entrained part of the plume within the well-mixed recirculation region; this is affecting results slightly. The new model development relating to how plumes that directly impact a building are modelled does not affect this study as all sources are on the roof.

## 6 References

- [1] Carruthers, D.J., McKeown, A.M., Hall, D.J. and Porter, S., 1999: *Validation of ADMS against wind tunnel data of dispersion from chemical warehouse fires*. In *Atmospheric Environment*, 33, 12, pp. 1937-1953.
- [2] Hall, D.J., Kukadia, V., Walker, S. and Marsland, G.W., 1995: *Plume dispersion from chemical warehouse fires*. BRE Client Report, CR 56/95.
- [3] Hall, D.J., Spanton, A.M., Dunkerley, F., Bennett, M. and Griffiths, R.F., 2000: *An intercomparison of AERMOD, ADMS and ISC dispersion models for regulatory applications*. Environment Agency Technical Report P362.
- [4] Stidworthy A, Carruthers D, Stocker J, Balis D, Katragkou E, and Kukkonen J, 2013: *MyAir Toolkit for Model Evaluation*. 15<sup>th</sup> International Conference on Harmonisation, Madrid, Spain, May 2013.
- [5] Thunis P., E. Georgieva, S. Galmarini, 2010: *A procedure for air quality models benchmarking*.  
[https://fairmode.jrc.ec.europa.eu/document/fairmode/WG1/WG2\\_SG4\\_benchmarking\\_V2.pdf](https://fairmode.jrc.ec.europa.eu/document/fairmode/WG1/WG2_SG4_benchmarking_V2.pdf)
- [6] David Carslaw and Karl Ropkins (2011). *openair: Open-source tools for the analysis of air pollution data*. R package version 0.4-7. <http://www.openair-project.org/>
- [7] Chang, J. and Hanna, S., 2004: *Air quality model performance evaluation*. *Meteorol. Atmos. Phys.* **87**, 167-196.